

# Sequencing Quality Control Report

Genomics Unit

February 19, 2015

## 1 Flowcell Information

Flowcell AC6BFYANXX  
Run Start 2015-02-16  
Read Length 50 paired end  
HiSeq Sequencing Kit TruSeq v4


Sequencer Software HiSeq Control Software 2.2.58  
Gerald version 1.8

## 2 Samples Information

LabID	Name	Index	NumberOfReadPairs
9273	ES 1	GCCAAT	113932317
9274	ES 2	CTTGTA	114681881

### 3 Quality Plots

**Sample 9273: ES 1**

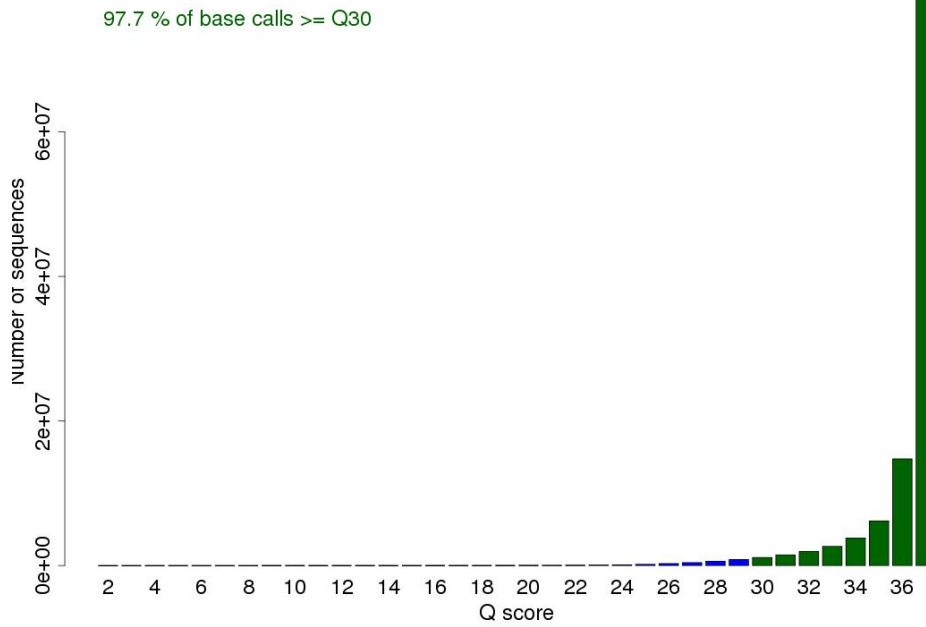

**Sample 9274: ES 2**

